

PROCEEDINGS OF SPIE

Photonics Applications in Astronomy, Communications, Industry, and High Energy Physics Experiments 2024

**Ryszard S. Romaniuk
Andrzej Smolarz
Waldemar Wójcik**
Editors

**27–30 June 2024
Lublin, Poland**

Organized by
Lublin University of Technology (Poland)
Warsaw University of Technology (Poland)
Photonics Society of Poland (Poland)
Polish Optoelectronics Committee of the Association of Polish Electrical Engineers (Poland)
Committee of Electronics and Telecommunications, Polish Academy of Sciences (Poland)

Published by
SPIE

Volume 13400

Proceedings of SPIE 0277-786X, V. 13400

SPIE is an international society advancing an interdisciplinary approach to the science and application of light.

Photonics Applications in Astronomy, Communications, Industry, and High Energy Physics Experiments 2024,
edited by Ryszard S. Romaniuk, Andrzej Smolarz, Waldemar Wójcik, Proc. of SPIE
Vol. 13400, 1340001 · © 2024 SPIE · 0277-786X · doi: 10.1117/12.3058889

Proc. of SPIE Vol. 13400 1340001-1

The papers in this volume were part of the technical conference cited on the cover and title page. Papers were selected and subject to review by the editors and conference program committee. Some conference presentations may not be available for publication. Additional papers and presentation recordings may be available online in the SPIE Digital Library at SPIDigitalLibrary.org.

The papers reflect the work and thoughts of the authors and are published herein as submitted. The publisher is not responsible for the validity of the information or for any outcomes resulting from reliance thereon.

Please use the following format to cite material from these proceedings:

Author(s), "Title of Paper," in *Photonics Applications in Astronomy, Communications, Industry, and High Energy Physics Experiments 2024*, edited by Ryszard S. Romaniuk, Andrzej Smolarz, Waldemar Wójcik, Proc. of SPIE 13400, Seven-digit Article CID Number (DD/MM/YYYY); (DOI URL).

ISSN: 0277-786X
ISSN: 1996-756X (electronic)

ISBN: 9781510685789
ISBN: 9781510685796 (electronic)

Published by
SPIE
P.O. Box 10, Bellingham, Washington 98227-0010 USA
Telephone +1 360 676 3290 (Pacific Time)
SPIE.org
Copyright © 2024 Society of Photo-Optical Instrumentation Engineers (SPIE).

Copying of material in this book for internal or personal use, or for the internal or personal use of specific clients, beyond the fair use provisions granted by the U.S. Copyright Law is authorized by SPIE subject to payment of fees. To obtain permission to use and share articles in this volume, visit Copyright Clearance Center at copyright.com. Other copying for republication, resale, advertising or promotion, or any form of systematic or multiple reproduction of any material in this book is prohibited except with permission in writing from the publisher.

Printed in the United States of America by Curran Associates, Inc., under license from SPIE.

Publication of record for individual papers is online in the SPIE Digital Library.

SPIE. DIGITAL LIBRARY
SPIDigitalLibrary.org

Paper Numbering: A unique citation identifier (CID) number is assigned to each article in the Proceedings of SPIE at the time of publication. Utilization of CIDs allows articles to be fully citable as soon as they are published online, and connects the same identifier to all online and print versions of the publication. SPIE uses a seven-digit CID article numbering system structured as follows:

- The first five digits correspond to the SPIE volume number.
- The last two digits indicate publication order within the volume using a Base 36 numbering system employing both numerals and letters. These two-number sets start with 00, 01, 02, 03, 04, 05, 06, 07, 08, 09, 0A, 0B ... 0Z, followed by 10-1Z, 20-2Z, etc. The CID Number appears on each page of the manuscript.

Contents

vii	Conference Committee
ix	Introduction

CONFERENCE OVERVIEW

13400 02	Photonics applications and web engineering: WILGA 2024 (Invited Paper) [13400-36]
----------	--

BIOMEDICAL APPLICATIONS

13400 03	Thin-layer chromatography image segmentation for toxicological studies (Invited Paper) [13400-1]
13400 04	Mueller matrix and laser induced imaging of the myocardium histological sections in the diagnosis of long-term consequences of COVID19 [13400-3]
13400 05	Polarization mapping of optical anisotropy architectonics laser induced images in monitoring biological tissue necrosis [13400-6]
13400 06	3D polarimetry of laser induced speckle fields for phase detection thyroid gland polycrystalline structure and traumatic necrosis of human internal organs [13400-7]
13400 07	Automated optical system of integrated photostimulation of the human nervous system [13400-8]
13400 08	Layer-by-layer phase scanning of polycrystalline blood facies laser induced images for determination thyroid gland cancer and tissues injury necrosis [13400-9]
13400 09	Polarization-phase laser induced and holographic reconstruction of blood facies polycrystalline architectonics in the diagnosis of long-term consequences of COVID-19 [13400-11]
13400 0A	Neural network method for assessing the effectiveness of the formation of pathological and keloid scars [13400-12]
13400 0B	The method of pyramid contour Q-transformation of biomedical images [13400-17]
13400 0C	Simulation modeling of conversion processes of polarized optical radiation in biological tissue [13400-19]
13400 0D	Physical modeling of output cascades and terminal devices of laser medical equipment with a rectangular cross-section of the output optical beam (Invited Paper) [13400-22]

- 13400 OE **High-performance information technology for processing large datasets and biomedical images to improve the accuracy of computer-aided decision support systems (Invited Paper)** [13400-25]
- 13400 OF **Digital ultrasound image processing method with an example of a hip joint condition study (Invited Paper)** [13400-26]
- 13400 OG **Human-beta-defensin-1, ferritin, and interleukin-6 in a mathematical model for predicting the effectiveness of anti-tuberculosis treatment** [13400-29]
- 13400 OH **Automated splint design system for nasal surgery** [13400-33]
- 13400 OI **Application of optical methods for measuring physiological parameters in the construction of telemedicine systems for the diagnosis of infants and children** [13400-34]

MATERIALS, METROLOGY, AND IMAGE PROCESSING

- 13400 OJ **Transformers in image super-resolution: a brief review** [13400-4]
- 13400 OK **Modern programming technologies in the tasks of identification and classification of military aircraft using machine learning algorithms** [13400-13]
- 13400 OL **Vacuum nanoscale carbon coatings** [13400-15]
- 13400 OM **Regression method for inverse correlation filters design for objects recognition** [13400-16]
- 13400 ON **Modified parallel-hierarchical transformation algorithm for processing of optical imaging** [13400-18]
- 13400 OO **Method of combined vector normalization of 3-D objects** [13400-20]
- 13400 OP **Image processing based on hybrid semi-supervised learning** [13400-28]
- 13400 OQ **Results of studies on the emissivity of metal powder for implementing an intelligent control approach in additive manufacturing** [13400-30]
- 13400 OR **Re-identification of people in a video stream based on a Kalman filter** [13400-31]

COMPONENTS, COMMUNICATIONS, AND ICT FOR PHOTONICS

- 13400 OS **FPGA matrix multiplication with resource optimization and constraints (Invited Paper)** [13400-2]
- 13400 OT **Method to improve information security in fiberoptic systems and networks** [13400-5]

- 13400 OU **Precision control model for chaotic laser generation in optical communication and laser measurement systems** [13400-10]
- 13400 OV **Monitoring of the road surface using a fiber sensor based on a fiber Bragg grid (Invited Paper)** [13400-14]
- 13400 OW **Application of optoelectronic components in intelligent systems** [13400-21]
- 13400 OX **Innovative approaches to creating digital content for programs in photonics and optoelectronics** [13400-23]
- 13400 OY **Modelling a modified parallel-hierarchical transformation algorithm for laser beam image processing** [13400-32]
- 13400 OZ **Evaluating machine learning-based routing algorithms on various wireless network topologies** [13400-35]

Conference Committee

Conference Chairs

Ryszard S. Romaniuk, Warsaw University of Technology (Poland)
Andrzej Smolarz, Lublin University of Technology (Poland)
Waldemar Wójcik, Lublin University of Technology (Poland)

Program Committee

Waldemar Wójcik, Lublin University of Technology (Poland)
Ryszard S. Romaniuk, Warsaw University of Technology (Poland)
Andrzej Smolarz, Lublin University of Technology (Poland)
Piotr Kisała, Lublin University of Technology (Poland)
Andrzej Kotyra, Lublin University of Technology (Poland)
Paweł Komada, Lublin University of Technology (Poland)
Zbigniew Omiotek, Lublin University of Technology (Poland)
Sławomir Ciężczyk, Lublin University of Technology (Poland)
Jacek Kuszniar, Białystok University of Technology (Poland)
Krzysztof Pozniak, Warsaw University of Technology and CERN (Poland)
Sergii Pavlov, Vinnitsya National Technical University (Ukraine)
Volodymyr Lytvynenko, Kherson National Technical University (Ukraine)
Oleh Avrunin, Kharkov National Technical University (Ukraine)
Nataliia Savina, National University of Water and Environmental Engineering (Ukraine)
Nataliia Zabolotna, Vinnitsya National Technical University (Ukraine)
Saule Rakhmetulina, D. Serikbayev East Kazakhstan Technical University (Kazakhstan)
Saule Smailova, D. Serikbayev East Kazakhstan Technical University (Kazakhstan)
Aliya Kalizhanova, Institute of Information and Computational Technologies (Kazakhstan)
Orken Mamyrbayev, Institute of Information and Computational Technologies (Kazakhstan)
Krzysztof Skorupski, Lublin University of Technology (Poland)

Program Committee

Andrzej Smolarz, Lublin University of Technology (Poland)
Damian Harasim, Warsaw University of Technology (Poland)
Róża Dzierżak, Lublin University of Technology (Poland)
Żaklin Grądz, Lublin University of Technology (Poland)
Jacek Majcher, Lublin University of Technology (Poland)

Introduction

Wilga Symposium used to be a multidisciplinary and multi-conference meeting of young scientists and engineers. Wilga meetings and workshops aimed primarily at Ph.D. students and freshly graduated researchers. It was organized since 1995 two times a year, featuring winter and spring/summer editions. Since 2002 Wilga papers are published in the Proceedings of SPIE. The major topical track of Wilga used to be Photonics Applications. This track was extended to related fields and embraced coupling of photonics to other subjects like mechatronics, optoelectronics, laser technologies, electronics, communications, image processing, and information technologies.

Due to this coupling more complex and bigger systems were considered with core solutions containing photonics. Wilga meetings were also related with other optical, optoelectronic, and photonic conferences organized locally but of international extent. These conferences were Optical Fibers and Their Applications, with papers published in Proceedings of SPIE since 1986, and Laser Technology with papers published in Proceedings of SPIE since 1987.

The WILGA winter and summer meetings on Photonics Applications were initiated by the PERG-ELHEP Research Laboratory at the Institute of Electronic Systems of Warsaw University of Technology, Poland in 1995. The meetings started to be numbered with the winter edition of 1998, thus this year the summer edition 2024 was the 52nd jubilee. The Photonics Engineering Research Group joined forces with the Electronics Laboratory for High Energy Physics Experiments Laboratory at IES WUT to start organizing international research meetings on the integration of photonics, electronics, and mechatronics in demanding advanced applications. To start a new series of conferences is not always easy. In this particular case, the factors that strongly supported the beginning process for these meetings had domestic and international cooperation with young research teams, friendly cooperation with key research organizations, international support from SPIE and IEEE, and domestic support from the Association of Polish Electrical Engineers.

The essential factor was involvement of the initiating laboratory as well as international cooperation from laboratories like Deutsches Elektronen Synchrotron DESY in Hamburg, Germany; CERN in Geneva, Switzerland; Fermilab near Chicago, USA; and later with TJNAF in Newport News, USA; ITER in Cadarache, France; FAIR/GSI in Darmstadt, Germany; etc. Since 2002 SPIE – The International Society for Optics and Photonics generously agreed to support the WILGA Symposium and publish the proceedings of these young researchers' meetings in the Proceedings of SPIE. The volumes were published annually from joint winter and summer editions of WILGA Symposium under the common title Photonics Applications in Astronomy, Communications, Industry, and High Energy Physics Experiments.

For a number of years, SPIE has generously funded awards for the best student presentation in WILGA. WILGA, the Photonics Applications Symposium, was held at a small village resort owned by Warsaw University of Technology, Poland and is located 50 kilometres up the Vistula River from Warsaw. During the 25 years of numbered editions of the WILGA Symposium on Photonics Application, the meetings gathered more than 6000 young researchers, among them the majority of Ph.D. students active in Photonics, who published more than 2000 papers in Proceedings of SPIE, and 1000 papers elsewhere.

Since 2022 Wilga Symposium was intentionally moved to Lublin, with the major organizers residing in the Lublin University of Technology. The WILGA 2021, 2022, and 2024 Symposia on Photonic Applications gathered, partly via virtual links, a significant number of scholars from Ukraine who submitted content for publication which is also reflected in this volume of Proceedings. Some of Ukrainian scholars were able to come personally to Lublin which is a beautiful academic city located in eastern part of Poland not far away from the Ukrainian border.

The topical areas of these recent Wilga meeting were divided to three main sections: biomedical applications; materials, metrology, and image processing; components, communications, and ICT for photonics. These areas were discussed with participants to promote cooperation with Ukrainian research institutions and individual researchers. The editors would like to thank all Wilga Symposium participants, who made also this SPIE volume of proceedings possible.

Andrzej Smolarz
Ryszard S. Romaniuk
Waldemar Wójcik

Digital ultrasound image processing method with an example of a hip joint condition study

Yosyp Bilynsky^a, Anzhelika Starover^b, Artem Huralnyk^c, Liudmyla Husak^c, Oleksandr Poplavskyi^d, Mariana Kovtoniuk^e, Marta Tarczyńska^f, Krzysztof Gawęda^f, Dinara Ussipbekova^g
^aVinnitsia National Technical University, 95 Khmelnytske Shose, Vinnitsia, Ukraine; ^bNational Pirogov Memorial University, 95 Khmelnytske Shose, Vinnitsia, Ukraine; ^cVinnitsia Trade and Economic Institute DTEU, 58 Soborna str., Vinnitsia, Ukraine; ^dKyiv National University of Construction and Architecture, Kyiv, Ukraine; ^eVinnitsia Mykhailo Kotsiubynskyi State Pedagogical University, Ostrozhskogo street 32, Vinnitsa, 21100, Ukraine; ^fArthros Med Ctr, Chodzki 31 St, PL-20090 Lublin, Poland; ^gDepartment of information communication technologies, Kazakh National Medical University named after S.D. Asfendiyarov, Almaty 050000, Kazakhstan

ABSTRACT

Medical and biological images have different physical natures. A person-operator can perceive them in different ways. Therefore, an important task is the adaptation of the image processing process to a specific user, that is, to a narrow task that is solved by the consumer of information. It is often not enough to present an object to an observer with the help of an ideal display system, since the information required for image analysis in order to search and identify objects, the determination of various quantitative characteristics can be manifested only as a result of digital processing. Based on the above, the paper proposes an automated method for extracting the contours of ultrasound images using the example of studying the state of the hip joint. This method makes it possible to construct conventional lines on the image of the hip joint in an automated mode with minimal expenditure of resources and subsequently to calculate the values of certain angular indicators, and using known methods of studying the condition of the hip joint, to estimate its degree of dysplasia. By automating the process, the reliability of diagnostics can be increased.

Keywords: image processing, modeling, filtering, contrast, selection of the contour on the image, dysplasia, condition of the hip joint, ultrasound, conditional lines.

1. INTRODUCTION

The problem of the consequences of diseases of the musculoskeletal system occupies a leading place in modern pediatric orthopedics and traumatology. Among the deformities of the musculoskeletal system, the most common is hip dysplasia, which is an abnormality of the hip joint when the socket part does not sufficiently cover the ball part, which leads to an increased risk of dislocation of the joint. Dysplasia of the hip joint is a congenital disorder in the structure of the hip joint that occurs due to improper development of the joint. The disease develops when the joint has not formed normally, so it does not work properly.

3% of children are diagnosed with hip dysplasia after birth. Pathology is diagnosed 6 times more often in girls. Therefore, already in the first hours of life, the child must be examined by a pediatric orthopedic traumatologist. Therefore, in order to prevent the negative consequences of the pathology, it is necessary to diagnose and start treatment in time.

A preliminary diagnosis of dysplasia is sometimes made in the first hours after birth. The doctor must examine the newborn to make sure that everything is fine with the baby. Palpation and examination of the baby is carried out after feeding in a calm environment.

To confirm the diagnosis, an additional study is prescribed, which includes such procedures as ultrasound examination (ultrasound) (to determine the cause and localization of disorders), radiography (for adults and children over one year), computer tomography (to assess the state of the bone-ligamentous apparatus).

The use of the X-ray method is associated with radiation exposure, which does not allow its use in children under the age of three months. In addition, the radiograph does not show non-ossified structures - parts of the head of the femur, the

*e-mail: yosyp.bilynsky@gmail.com

roof of the acetabulum, which make up the majority of these anatomical formations in children of the first year of life. The consequence of this is the impossibility of detecting disorders of enchondral formation, which is sometimes the main manifestation of hip dysplasia^{1,2,3}.

Although ultrasound equipment is widely available, proper practice and experience are required to obtain accurate ultrasound results. Despite the fact that the experience of using hip joint ultrasound in pediatrics is growing, this study may not always be accessible and convenient, and only an experienced doctor can make a reliable diagnosis based on visual observation and classify the type of dysplasia according to known methods^{4,5}.

Today, the main methods of ultrasound assessment of the state of the hip dysplasia are the methods of Graf, Rosendahl, Harke and Morin, Terjesen, and Dahlström. But they do not have a high reliability of diagnosis, since they are performed manually^{6,7}. The result of the diagnosis mainly depends on the doctor's qualifications, since during the examination there may be an incorrect visualization of the anatomical landmarks of the hip joint, made when the child is in the wrong position⁸. This leads to the impossibility of correct measurement of angular indicators, and there is also a sufficiently large error that occurs when manually determining angles on an ultrasound image noisy with speckle noise⁹.

Since the bone system is not formed in small children, a special marking method is used for decoding. Conventional lines are drawn on pictures taken in frontal projection to obtain angles, the size of which allows determining the degree of joint deformity. Based on the received data, the presence of violations is determined.

Today, in connection with the emergence of new computer technologies, it is possible to automate this process and classify existing dysplasia.

To fulfill the above and the goal set in this work by developing a mathematical model for automating the process of contour selection and drawing conventional lines on the ultrasound image of the hip joint.

2. DIGITAL PROCESSING OF AN ULTRASOUND IMAGE ON THE EXAMPLE OF A STUDY OF THE STATE OF THE HIP JOINT

Extraction of contours and image filtering is a very important part for high-precision medical operations, such as operations on the heart and brain of a person, where maximum precision of actions and understanding of exactly where certain medical procedures need to be done in order not to harm the patient are required. This also applies to ultrasound images. Therefore, for the automated application of conventional lines on the ultrasound image of an object, it is necessary to highlight the contour of this object.

The simplest method of extracting the primary contour of the image is threshold processing, if the intensity of a pixel is above a certain threshold, then the pixel takes the value of a logical unit, if it is below the threshold, then the logical value of zero. But this approach can be applied only for images with a uniform background, and the intensity values of the objects take the same values throughout the image. The studied ultrasound images, as a rule, do not meet the above criteria, have a heterogeneous background and noise, so this method will not give the necessary satisfactory results¹⁰.

The best results are given by operators based on the gradient contour selection method. These operators differ in window size, weighting factors, and registration methods¹¹.

With processed ultrasound images, it is difficult to distinguish the contour using such methods, since the magnitude of the boundary gradient and noise practically have the same value. In addition, the contour line obtained by this method, although it is continuous, is indistinct and blurred, which practically makes it impossible to automatically select objects and calculate their geometric parameters.

Today, the optimal Kanni detector¹² is widely used for image contour selection. The Canny edge detector algorithm is not limited to computing the gradient of a smoothed image. Only the maximum points of the image gradient remain in the contour, and the non-maximum points lying next to the border are removed. It also uses path direction information to eliminate points near the boundary and not break the boundary itself. The scale of the Gaussian sigma determines the amount of noise suppression: the wider the Gaussian, the greater the smoothing effect. But increasing this scale reduces the accuracy of boundary localization. Since the detector consists of several algorithms (LoG and Canny), the computational costs increase dramatically.

The advantages of the Canny detector are high resistance to noise due to the use of the Gaussian method, which gives a better quality of image segmentation, and also remains sensitive to low-contrast images. The main disadvantages of

detectors of this type are the high complexity of calculations and long processing time, the selection of spurious contours, with slight changes in intensity, the detectors do not work, since many spurious contours appear in the image, and the small value of the gradient does not allow you to quickly set the appropriate threshold level and identify the change intensity as a contour²⁴.

The paper proposes an approach that involves the use of global binarization of images using the Otsu's method. This method is based on automatically calculating the threshold image, or reducing the gray image to a binary image. The algorithm assumes that the image contains two classes of pixels, the following bi-modal histogram: foreground pixels and background pixels. Then the optimal threshold separating the two classes is calculated so that their combined range (cluster variance) is minimal or equal (because the sum of pairwise squared distances is constant) so that their intercluster variance is maximal. Therefore, Otsu's method is an approximate one-dimensional discrete analogue of Fisher's discriminant analysis. This method is the best way to find a global image threshold and is self-explanatory and suitable for most cases where a global image threshold is desired. The advantages of Otsu's method are ease of implementation, adaptation to various images by choosing the optimal threshold, and fast execution time. The disadvantages of the method are that the image is sensitive to noise. It can be segmented for only one purpose, when the ratio of the size of the object to the background is large, and the variance function between classes can show double or multiple peaks¹³. Therefore, for further work with such an image, it is necessary to select a fragment of the image of the hip and filter the image in order to reduce the noise component. The recorded ultrasound image of the hip joint is shown in Figure 1a.

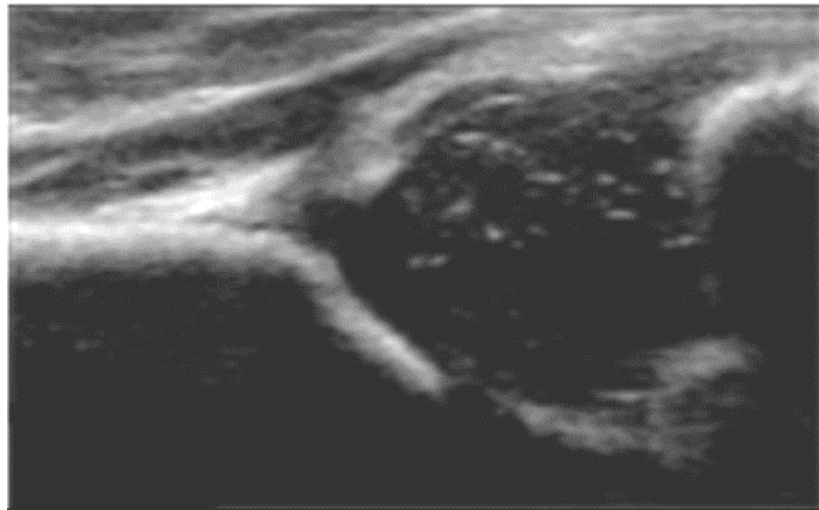


Figure 1. Ultrasound image of the hip joint.

Today, there are two main approaches aimed at suppressing noise in ultrasound images: frame-by-frame averaging and post-processing. Each of these approaches has disadvantages:

- frame averaging reduces the real frequency of frame changes, since the image obtained as a result of processing is a superposition of several processed frames. Therefore, the image of moving objects, when several frames are superimposed on each other, can be indistinct, blurred;
- the result of the post-processing filter is a possible loss of detail and an increase in processing time, although the "readability" of the processed image is better than that of the original¹⁴.

Since the hip joint image can be considered static and in order to simplify the further processing algorithm, the image filtering of the first approach was used, namely, the median filter was applied. This filter is usually used for filtering mainly impulse noises and has become widespread due to its reliability and the ability to preserve the contour. The median filter uses the median value of the pixel intensity within an area, thus creating less blur in images than other filters. This filter also requires the user to set the size of the sliding window. For this algorithm, different sizes of image processing windows 3, 5, 7 and 9 were used. In Fig. 2 shows a selected fragment of the hip joint image processed by a median filter with a window size of 3×3 .

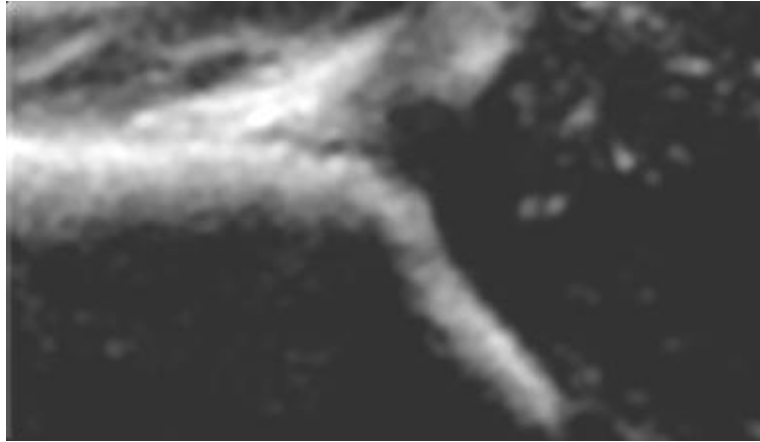


Figure 2. Selected fragment of the hip image, proves with a 3x3 window.

We will perform linear contrast of the hip joint image (Fig. 3)¹⁵. Such contrast is used to match the dynamic range of the input image signal and the dynamic range of brightness of the display device. If 1 byte (8 bits) of the memory device is allocated for the digital value of each image reading, then the input or output signals can acquire one of 256 values. When comparing two images (input and output) of the hip, a much better visual quality of the processed image is established.



Figure 3. Linear contrast of hip image.

Using the Otsu's method, we will obtain a binary image of a fragment of the hip joint (Fig. 4a). The histogram of such an image contains only two types of pixels - with zero and maximum brightness (Fig. 4b).



a)



b)

Figure 4. Binary hip image with Otsu's method (4a), histogram image (4b)

The use of such a hip joint image significantly simplifies the selection of its contour and does not require the use of complex methods. In fig. 5a shows the contour image of the hip using the Roberts operator. At this stage of the algorithm, any known contour selection operators can be used. In fig. 5b shows the contoured image of hip.

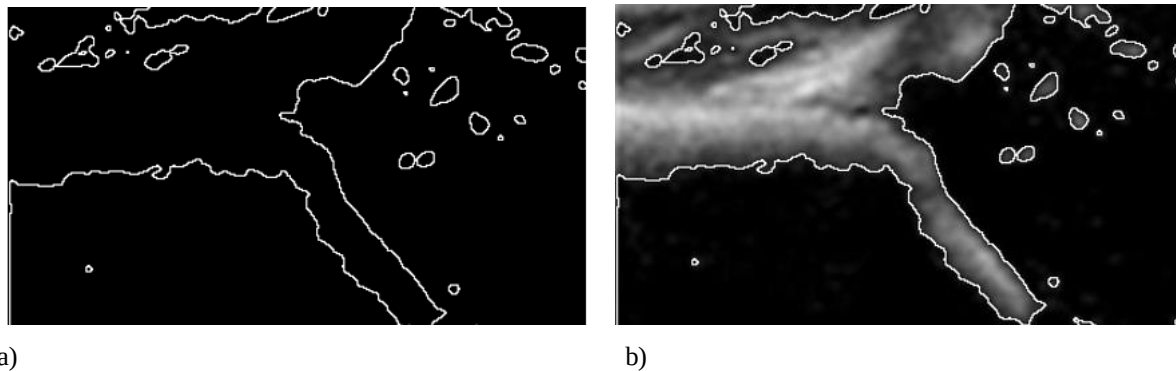


Figure 5. Contour image of hip joint with Roberts operator (a), contoured image (b)

If the information obtained on the basis of the image in Fig. 5 is not enough, then, using the tool for selection of rectangular areas on the image, you can select areas of the image in which conditional lines or points of this object will be formed on the image. In our case, it concerns the bony triangle of the acetabulum and the roof of the cartilage to assess the state of the hip joint. For this purpose, the Rectangular Marquee or Polygonal Lasso tool is used, which is widely available in graphic editors. In fig. 6 shows an example of a hip joint image with highlighted areas.

Using the data array of the contour lines of the selected areas and known approximation methods, such as the method of least squares, and linear interpolation, it is possible to select the best polynomial trend lines as shown in Fig. 7. Analogously, polynomial curves can be obtained if necessary.

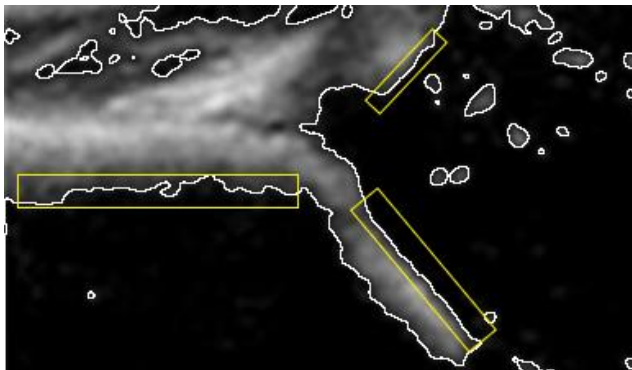


Figure 6. Hip joint image with selected areas

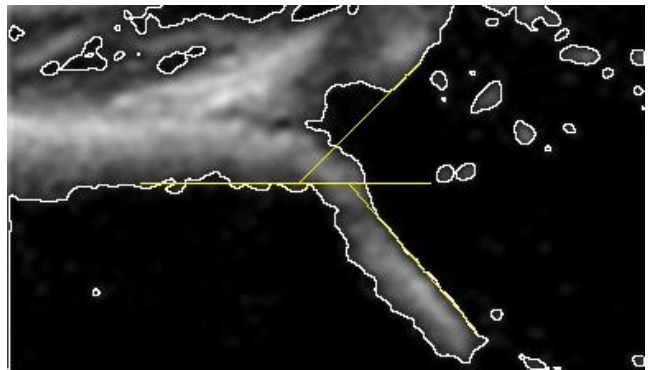


Figure 7. Applying conventional lines on the image of the hip joint

3. CONCLUSION

The paper proposes an automated method of processing ultrasound images using the example of a child's hip joint, which makes it possible to improve the image itself, highlight hidden objects, and determine their geometric parameters. The method includes such steps as capturing a specific region of the hip joint, performing image filtering and linear contrast, and converting the image to binary using the Otsu operator. This makes it possible to obtain an ideal contour and subsequently contour the object in the image, draw conditional lines and calculate angular indicators according to known methods.

The proposed detection method has not only sufficiently high accuracy, but also high speed with minimal use of resources.

REFERENCES

- [1] Asher MA. Screening for congenital dislocation of the hip, scoliosis, and other abnormalities affecting the musculoskeletal system. *Pediatr Clin North Am*;33:1335-53, (1986).
- [2] Bennet GC. Screening for congenital dislocation of the hip [Editorial]. *J Bone Joint Surg [Br]*;74: 643-4. (1992).
- [3] Aronsson DD, Goldberg MJ, Kling TF Jr, Roy DR. Developmental dysplasia of the hip. *Pediatrics* 1994;94(2 pt 1):201-8 [Published erratum in *Pediatrics* 94(4 pt 1):470, (1994).
- [4] Marks DS, Clegg J, al-Chalabi AN. Routine ultrasound screening for neonatal hip instability. Can it abolish late-presenting congenital dislocation of the hip? *J Bone Joint Surg [Br]* 76:534-8, (1994).
- [5] Hole KJ, Terjesen T, Tegnander A, Bredland T, Saether OD, Eik-Nes S. Ultrasound screening for hip dysplasia in newborns. *J Pediatr Orthop* 14:667-73, (1994).
- [6] Graf R. Hip ultrasonography. Basic principles and current aspects [German]. *Orthopade* 1997;26:14-24.
- [7] Rosendahl K, Markestad T, Lie RT. Congenital dislocation of the hip: a prospective study comparing ultrasound and clinical examination. *Acta Paediatr*;81:177-81, (1992).
- [8] Bilynsky Y, Nikolskyy A, Revenok V, Pogorilyi V, Smailova S, Voloshina O, Kumargazhanova S. Convolutional neural networks for early computer diagnosis of child dysplasia, *Informatyka, Automatyka, Pomiary W Gospodarce I Ochronie Środowiska*, 13(2) 56-63, (2023): <http://doi.org/10.35784/iapgos.3499>.
- [9] García Luis R. Luis-García, R. and C. Alberola-López. . World Scientific and Engineering Academy and Society (WSEAS). Hip joint segmentation from 2D ultrasound data based on dynamic shape priors. *Proceedings of the 4th WSEAS international conference on Electronics, control and signal processing* (2005).
- [10] Gonzales R, Wood R. *Digital image processing*. – M.: Technosphere,– 1072, (2005).
- [11] Canny J. A Computational Approach to Edge Detection, In *IEEE transactions on pattern analysis and machine intelligence*, vol. pami-8, no. 6, (1986).
- [12] Otsu N. A threshold selection method from gray-level histograms. *IEEE Trans. Sys., Man., Cyber.* 9 (1): 62—66.doi:10.1109/TSMC. 4310076. (1979).
- [13] Sivakumar R, Gayathri MK, Nedumaran D. Speckle filtering of ultrasound B-Scan Images - a comparative study between spatial and diffusion filters 2010 IEEE Conference on Open Systems (ICOS 2010) Published: (2010).
- [14] Abdul Nasi AS, Mashor MY, Mohamed Z. Modified Global and Modified Linear Contrast Stretching Algorithms: New Colour Contrast Enhancement Techniques for Microscopic Analysis of Malaria Slide Images, *Computational and Mathematical Methods in Medicine* (5):637360. (2012), DOI:10.1155/2012/637360.
- [15] Brittany Hillen, Photopea online image editor is a free Photoshop clone with advanced tools. *Digital Photography Review*. Archived from the original on December 4, 2020. Retrieved (June 14, 2019).